



Measurement of the accuracy of dental working casts using a coordinate measuring machine

Ispitivanje preciznosti radnih modela pomoću koordinatne merne mašine u stomatologiji

Michal Potran*, Branko Štrbac[†], Tatjana Puškar*, Miodrag Hadžistević[‡],
Janko Hodolić[†], Branka Trifković[‡]

*Department of Dentistry, Faculty of Medicine, University of Novi Sad, Novi Sad, Serbia; [†]Department of Production Engineering, Faculty of Technical Sciences, University of Novi Sad, Novi Sad, Serbia; [‡]Clinic for Prosthodontics, Faculty of Dental Medicine, University of Belgrade, Belgrade, Serbia

Abstract

Background/Aim. Dental impressions present a negative imprint of intraoral tissues of a patient which is, by pouring in gypsum, transferred extraorally on the working cast. Casting an accurate and precise working cast presents the first and very important step, since each of the following stages contributes to the overall error of the production process, which can lead to inadequately fitting dental restorations. The aim of this study was to promote and test a new model and technique for *in vitro* evaluation of the dental impression accuracy, as well as to assess the dimensional stability of impression material depending on the material bulk, and its effect on the accuracy of working casts. **Methods.** Impressions were made by the monophasic technique using the experimental master model. Custom trays with spacing of 1, 2 and 3 mm were constructed by rapid prototyping. The overall of 10 impressions were made with each custom tray. Working casts were made with gypsum type IV. Measurement of working casts was done 24 h later using a coordinate measuring machine. **Results.** The obtained results show that the working casts of all the three custom trays were in most cases significantly different in the transversal and sagittal planes in relation to the master model. The height of abutments was mainly unaffected. The degree of convergence showed certain significance in all the three custom trays, most pronounced in the tray with 3 mm spacing. **Conclusion.** The impression material bulk of 1–3 mm could provide accurate working casts when using the monophasic impression technique. The increase of the distance between abutment teeth influences the accuracy of working casts depending on the material bulk.

Key words: denture bases; denture design; elastomers; computer-aided design; sensitivity and specificity.

Apstrakt

Uvod/Cilj. Otisak predstavlja negativ intraoralnih tkiva, čijim se izlivanjem u gipsu njihova morfologija prenosi ekstraoralno na budući radni model. Sa laboratorijskog aspekta izrade zubnih nadoknada, izlivanje tačnog i preciznog radnog modela predstavlja prvi i veoma bitan korak, pošto svaka sledeća faza doprinosi daljem povećanju greške tokom izrade, što za krajnji ishod može imati neodgovarajuću zubnu nadoknadu. Cilj istraživanja bio je da se ispitaju novi model i tehnika za *in vitro* procenu preciznosti zubnih otisaka, kao i da se odredi uticaj količine otisnog materijala na dimenzionu stabilnost otisaka i preciznost izrade radnih modela. **Metode.** Za uzimanje otisaka korišćena je monofazna tehnika otiskivanja. Individualne kašike sa međuprostorom od 1, 2 i 3 mm napravljene su aditivnom tehnologijom za brzu izradu prototipova. Sa svakom kašikom napravljeno je po 10 otisaka. Radni modeli izliveni su u gipsu tipa IV. Merenje radnih modela vršeno je nakon 24 sata na koordinatnoj mernoj mašini. **Rezultati.** Rezultati pokazuju da radni modeli napravljeni pomoću sve tri individualne kašike u transverzalnoj i sagitalnoj ravni značajno odstupaju od glavnog dela modela. Visina patrljaka je u većini slučajeva bila kao na glavnom modelu. Step konvergencije pokazao je određena odstupanja samo kod kašike sa međuprostorom od 3 mm. **Zaključak.** Monofazna tehnika otiskivanja i otisni materijal debljine od 1 do 3 mm obezbeđuju izradu preciznih radnih modela. Rastojanje između zubnih patrljaka utiče na preciznost izrade radnih modela u zavisnosti od količine otisnog materijala.

Ključne reči: zubna proteza, baze; zubna proteza, oblikovanje; elastomeri; kompjutersko oblikovanje; osetljivost i specifičnost.

Introduction

Dental impressions present a negative imprint of intraoral tissues of a patient which is, by pouring in gypsum, transferred extraorally on the working cast. From the laboratory perspective of dental restorations manufacturing, casting an accurate and precise working cast presents the first and very important step, since each of the following stages contribute to the overall error of the production process and can lead to inadequately fitting of dental restorations¹.

Making an impression is a clinically challenging procedure which is influenced by numerous factors of the oral environment, as well as the properties of the material itself. Examining the factors that influence the accuracy of dental impressions can be conducted in two ways, by direct measurement of the impression, or by measurement of the appropriate working cast. Both methods have their advantages and limitations. The first method provides direct data about the condition of the impression material, thus avoiding superimposition of further errors. Limitations are related to the use of contactless measurement, which is affected by a small measurement field, software processing and adequate optical characteristics of the impression material²⁻⁴. The second method, measurement of the working casts, provides a wider range of possibilities regarding the measurement technique. Both contact and contactless measurement can be used, with ease of access for manipulation with measurement object⁵. Superimposition of errors, when casting a gypsum model, can be minimised by fixing the experimental conditions with equal casting protocols for all of the investigated dental impressions. Although making of the gypsum working cast prolongs the time and effort needed to obtain necessary data, it is a reference base for manufacturing of dental restorations and as such, provides better insight when assessing the discrepancies of future dental restorations.

Determination of accuracy of dental impressions requires a complex model that can replicate *in vivo* conditions of making of dental impressions, with the accuracy and precision of *in vitro* investigation. Earlier studies included a variety of models that consisted of custom blocks, cylinders, single or several abutment teeth and complete edentulous jaws of various materials⁵⁻¹¹. Regarding this, there is the need for a reliable experimental model, which combined with a corresponding measurement instrument, could overcome the difficulties of data interpolation between laboratory conditions and clinical practice. The two should complement each other, forming a complex model for data acquisition. From this point of view, the use of a coordinate measuring machine (CMM) was chosen due to the possibility of the accurate and precise three-dimensional (3D) measurement^{12, 13}.

Previous studies that investigated the influence of material bulk on the accuracy of working casts were conducted using a measurement microscope and included only two dimensional measurements¹⁴⁻¹⁶. Also, the models used consisted of one to several abutment teeth, while as to our knowledge, the influence of material bulk on partially edentulous dental arch model has not been made¹⁴⁻¹⁸. A more de-

tailed analysis requires a model more similar to the intraoral conditions, since the accuracy of impressions depends on the material bulk which changes with spacing between the remaining teeth¹⁹. The possibility of an independent 3D analysis by CMM for each of the segments of the working casts was considered to be an improvement compared to the previous studies.

Additionally to the previous studies, we aimed to incorporate another use of rapid prototyping (RP) technology in the field of dentistry. Making impressions with RP made custom trays is a new attempt to investigate the use of computer-aided design/computer-aided manufacturing (CAD/CAM) technology into a broader perspective of dental practice. The rapid prototyping technique was chosen with the aim of avoiding possible distortions of the material that can occur in standard acrylic custom trays, and providing a stable base for the impression material²⁰. Thus, the aim of this study was to promote and test a new model and technique for *in vitro* evaluation of the dental impression accuracy, as well as to assess dimensional stability of elastomeric impression material in reference to the material bulk, by examining working casts with CMM.

Methods

Measurement of the experimental master model and construction of custom trays

For the purpose of this study, an experimental metal master model which consisted of six abutment teeth was constructed. It presented the upper jaw with two central incisors, canines and first molars (Figure 1). Dimensions of the teeth were taken from literature and reduced by the amount of tooth substance expected to be removed with grinding²¹. The taper was set at 6°. The master model consisted of an assembly with machined components. Geometry of the master model and generation of computer numerical control machines (CNC) code was designed by the CAD/CAM system.



Fig. 1 – The experimental master model.

Measurement of the experimental master model was performed with the CMM (Contura G2, Carl Zeiss, Germany) equipped with a contact probe. Maximum permissible error for size measurement (MPE_E) of this CMM is $1.9 + L/330 \mu\text{m}$. The master model was measured five times and

the resulting mean values of parameters of measurement were calculated. Nominal dimensions of the CAD model were corrected using mean values and were subsequently used to create a custom tray model as a negative of the previous CAD model. Physical models of custom trays with 1, 2 and 3 mm spacings for the impression material, were constructed by rapid prototyping (Z310 plus, 3D Systems, USA). The powder used was gypsum based (zp 131), with a binder (zb 60) and two component epoxy resin as the filler (s5000), presented at Figures 2 and 3.



Fig. 2 – Custom trays with 1, 2 and 3 mm spacing made by rapid prototyping.

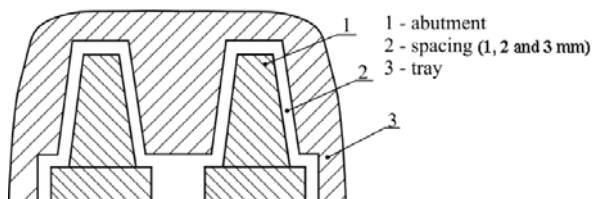


Fig. 3 – Custom tray seated on the top of the experimental master model.

Impression technique

Impressions were made using a monophasic technique with silicone addition. Due to the micromechanical retention of the impression material to a custom tray, which is the result of the successive layering technique of rapid prototyping, the tray adhesive was not used. The impression

material was automixed (Elite Hd + regular, Zhermack, Italy), working time was set to 60 sec. Making of impressions was conducted at room temperature (23°C), retention of the tray was done with the weight of 1 kg. Setting time was set at 10 min, overall of 10 impressions were made with each custom tray. Due to the expected viscoelastic recovery of the impression material, pouring of gypsum was delayed by 30 min. Working casts were made with the gypsum type 4 (Elite rock, Zhermack, Italy) and were allowed to set for 1 h before the impression was removed. Measurement of the working casts was done 24 h later on CMM.

Measurement of working casts on a coordinate measuring machine

Measurement of working casts was conducted under the same conditions as those of the master model. Inspection was conducted conformant to the new generation of product geometry specification (GPS) ²². This was based on the fact that the model consisted of geometric primitives (cones, cylinders and planes). Each geometric primitive was measured in a finite number of discrete points randomly arranged on the primitive surface. The measurement strategy of the cone (abutment) contained 100 measurement points, 50 points for measurement of cross-section plane between the cone and the cylinder (abutment and chamfer) and 50 for measurement of the cylinder (chamfer). The output of this measurement included the coordinates of all measurement points which were subsequently used to generate associative geometry of the primitives. Furthermore, the software analysis was used to determine all geometric characteristics (size, angle, form, orientation, location) according to the specification requirements.

Parameters, X_{1-3} and Y_{1-6} , represented the axial distances which were derived features from the cone. The axial distances were observed on the cross-sectional plane which passed through the base of the abutments. Parameters denoted as Z_{1-6} , were determined as the distance between two planes which limited the abutment vertically, while α_{1-6} represented the degree of convergence and was directly derived from the abutment measurement (Figure 4).

The presence of measurement uncertainty was disregarded due to the fact that all working casts were measured in

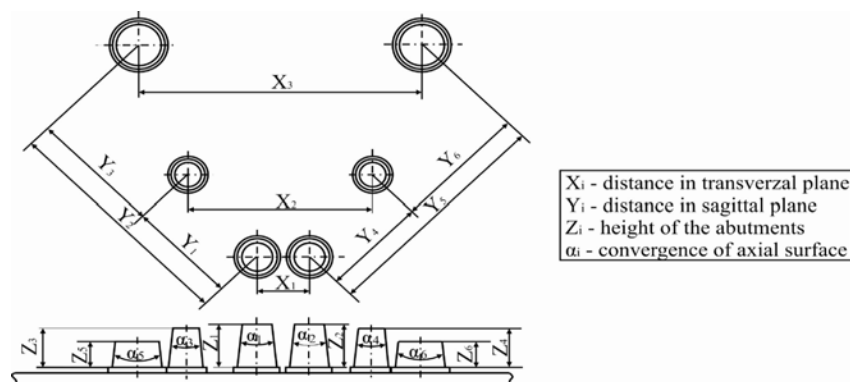


Fig. 4 – Parameters of measurement.

identical laboratory conditions: 24 h after casting, using the same position on machine table, by the same operator and using identical inspection strategies and stylus^{23,24}.

Statistical analysis

Statistical analysis of the results obtained from the measurement of the working casts was conducted by the two-sample *t*-test, which determined whether there was a statistically significant difference between the designated distances of working casts compared to the master model. One-way analysis of variance (ANOVA) was also conducted to establish if there were any significant differences in the results obtained by the type of custom tray for the considered parameters.

Results

The results of the two-sample *t*-test, with a 95% confidence interval, show that the working casts of all three custom trays were in most cases significantly different in transversal and sagittal plane in relation to the experimental master model (X_{1-3} , Y_{1-6}). The height of the abutments (Z_{1-6}) was mainly unaffected, while the degree of convergence (α_{1-6}) increased, especially in the working casts made by custom trays with 3 mm spacing. The results are presented in Table 1.

Most notable deviations for the first tray (T_1) were mea-

sured in X_3 (20 μm) for the transversal plane, Y_2 (27 μm) for the sagittal plane, Z_5 (-13 μm) for the height of the abutments and α_1 (-0.09°) for the convergence of axial surface. The dimensions of Z_{1-4} , Z_6 and α_3 , α_4 and α_6 showed no statistical significance in relation to the experimental master model.

Most pronounced deviations for the second tray (T_2) were measured in X_3 (22 μm) for the transversal plane, Y_2 (27 μm) for the sagittal plane, Z_5 (-15 μm) for the height of the abutments and α_1 (0.11°) for the convergence of axial surface. The dimensions of Y_1 , Y_5 , Z_{1-4} and α_6 showed no statistical significance in relation to the experimental master model.

The third tray (T_3) showed largest deviations in X_3 (36 μm) for the transversal plane, Y_2 (24 μm) for the sagittal plane, Z_5 (-7 μm) for the height of the abutments and α_1 (-0.18°) for the convergence of axial surface. Dimensions of Y_1 , Y_5 , Y_6 , Z_{1-6} showed no statistical significance in relation to the experimental master model.

Analysis of variance with a 95% confidence interval showed that the type of tray did not have any significant influence ($p > 0.05$) on the parameters of measurement, except for the X_3 and α_{1-6} . ($p < 0.05$) Therefore, with respect to α_{1-6} and X_3 , the third tray yielded the results which were significantly different from the first two trays. The presentation and graphical comparison of the results are shown in Figures 5 and 6.

Table 1

Results of the measurement														
Distance	Master (mm)	Mean (mm)			Standard deviation (μm)			Difference (μm)			<i>t</i> -test <i>p</i>			ANOVA <i>p</i>
		T_1	T_2	T_3	T_1	T_2	T_3	T_1	T_2	T_3	T_1	T_2	T_3	
X_1	8.507	8.521	8.522	8.52	1.74	2.19	1.94	14	15	13	0.00	0.00	0.00	0.29
X_2	30.002	30.015	30.012	30.012	3.99	5.63	6.66	13	10	10	0.00	0.00	0.00	0.58
X_3	46.015	46.035	46.037	46.051	10.9	13.5	11	20	22	36	0.00	0.00	0.00	0.02
Y_1	18.144	18.150	18.148	18.147	3.4	5	2.89	6	4	3	0.00	0.10	0.07	0.18
Y_2	42.051	42.078	42.078	42.075	7.27	8.36	6.92	27	27	24	0.00	0.00	0.00	0.82
Y_3	24.364	24.380	24.383	24.384	4.28	4.52	4.27	16	19	20	0.00	0.00	0.00	0.32
Y_4	18.319	18.326	18.326	18.323	4.32	4.15	3.65	7	7	4	0.00	0.00	0.01	0.06
Y_5	42.149	42.164	42.161	42.161	7.28	19.4	16	15	12	12	0.00	0.12	0.08	0.93
Y_6	24.277	24.283	24.287	24.282	4.43	9.15	13.5	6	10	5	0.00	0.01	0.27	0.57
Z_1	7.506	7.504	7.502	7.509	9.5	4.9	8.6	-2	-4	3	0.55	0.06	0.33	0.2
Z_2	7.507	7.507	7.506	7.512	8.5	6.2	8.9	0	-1	5	0.82	0.61	0.35	0.5
Z_3	6.923	6.926	6.926	6.924	10.4	7.8	11.7	3	3	1	0.20	0.28	0.71	0.92
Z_4	6.926	6.927	6.919	6.921	7.8	11.7	9.7	1	-7	-5	0.13	0.17	0.24	0.33
Z_5	5.000	4.487	4.485	4.493	8.16	8.66	11.5	-13	-15	-7	0.00	0.00	0.17	0.24
Z_6	4.497	4.491	4.486	4.493	9.41	9.87	13.7	-6	-11	-4	0.09	0.01	0.44	0.46
Angle	Master (°)	Mean (mm)			Standard deviation (mm)			Difference (°)			<i>t</i> -test <i>p</i>			ANOVA <i>p</i>
		T_1	T_2	T_3	T_1	T_2	T_3	T_1	T_2	T_3	T_1	T_2	T_3	
α_1	11.848	11.759	11.733	11.667	0.017	0.031	0.041	-0.09	-0.11	-0.18	0.00	0.00	0.00	0.00
α_2	11.827	11.779	11.721	11.697	0.028	0.023	0.071	-0.05	-0.11	-0.13	0.00	0.00	0.00	0.00
α_3	11.753	11.795	11.743	11.656	0.052	0.055	0.066	0.04	-0.01	-0.09	0.06	0.00	0.00	0.00
α_4	11.795	11.766	11.745	11.669	0.036	0.051	0.043	-0.03	-0.05	-0.13	0.05	0.02	0.00	0.00
α_5	11.912	11.851	11.843	11.747	0.051	0.079	0.087	-0.06	-0.07	-0.16	0.01	0.04	0.00	0.02
α_6	11.793	11.828	11.751	11.647	0.071	0.057	0.136	0.03	-0.04	-0.14	0.19	0.08	0.02	0.00

For abbreviations see Figure 4.

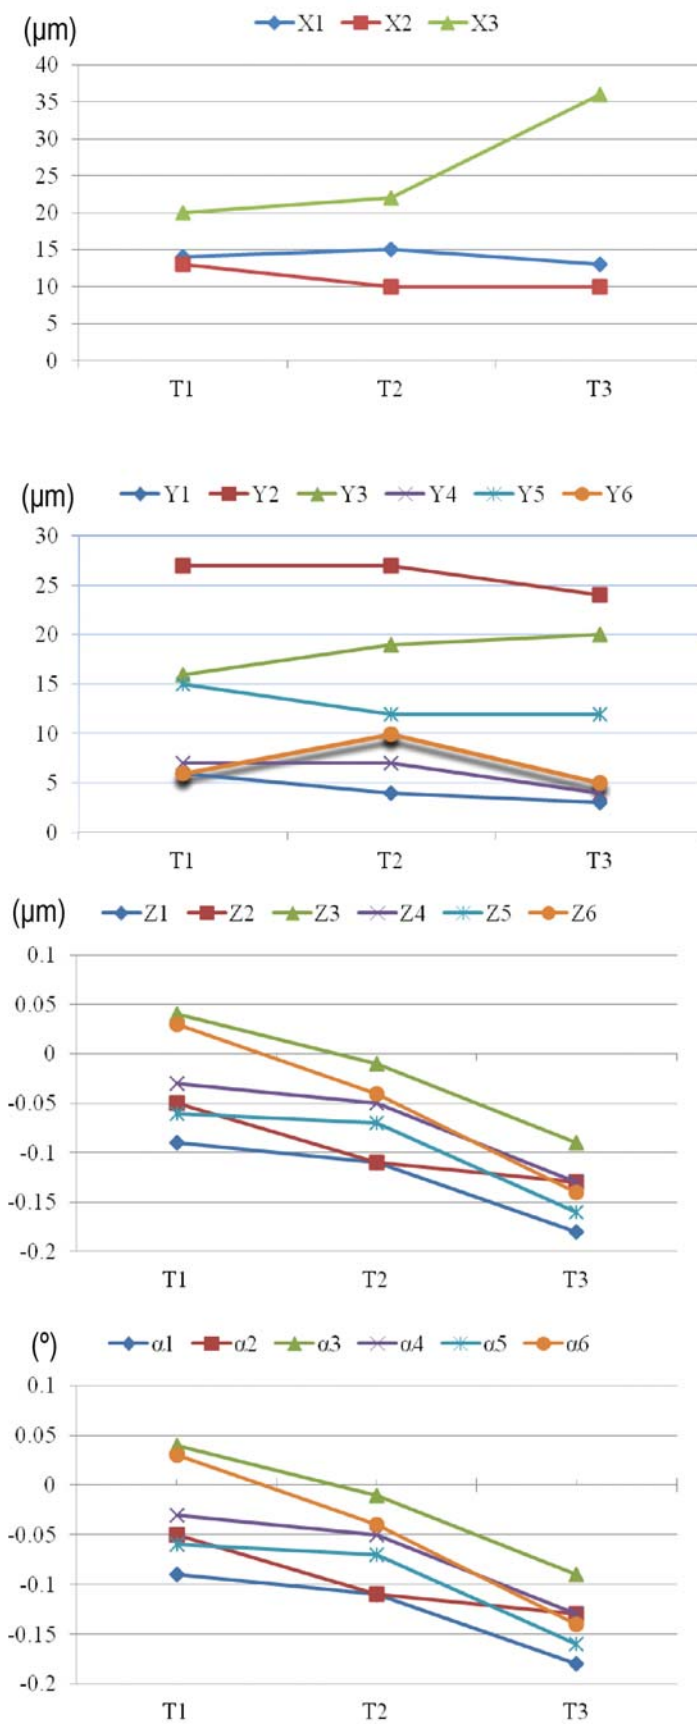


Fig. 5 – Comparison of distance in transversal (X₁₋₃), sagittal plane (Y₁₋₆), height of the abutments (Z₁₋₆) and convergence of axial surface (α₁₋₆) between custom impression trays and the master model.

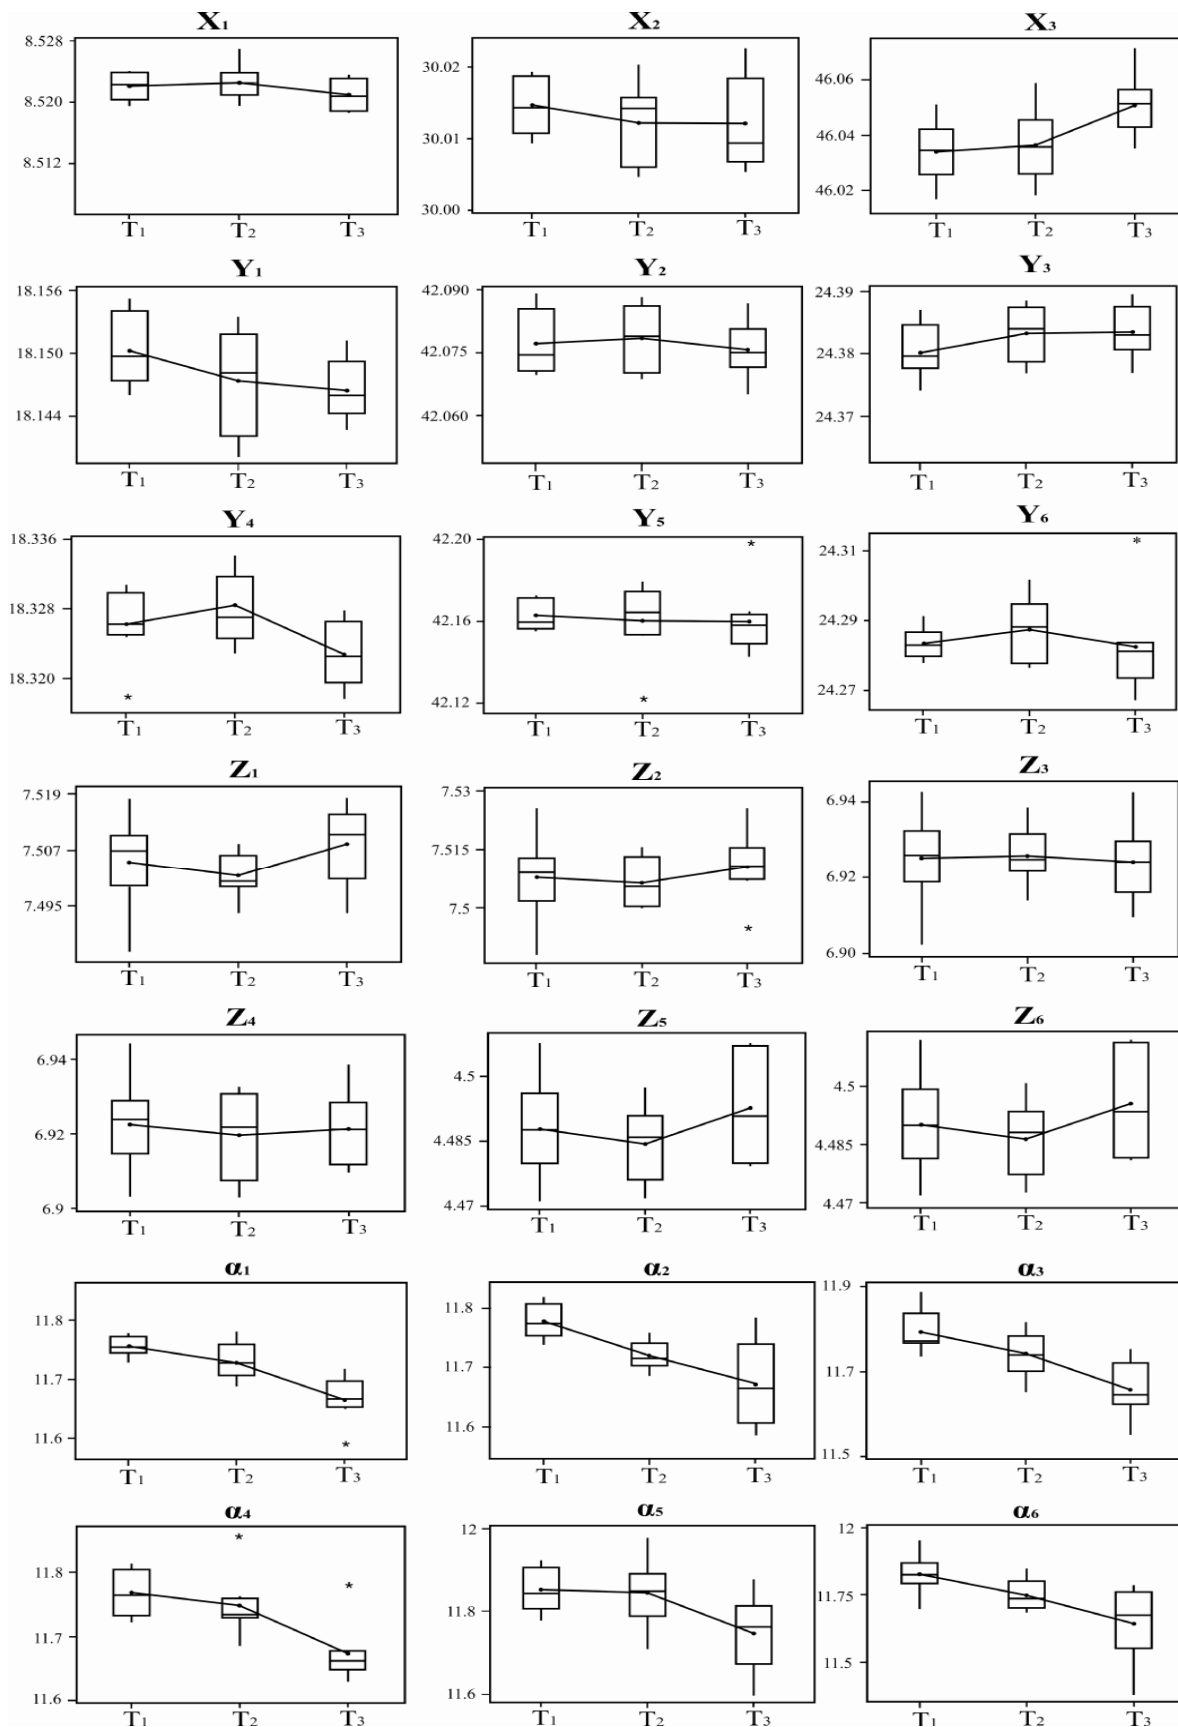


Fig. 6 – Mutual comparison of custom impression trays with 1, 2 and 3 mm spacing (T₁, T₂ and T₃, respectively).

Discussion

The results of this study show that both the experimental master model and the technique used for making the dental impressions have proven to be a reliable method for assessment of the accuracy of dental impression materials. Working casts obtained from all the three custom trays were, in most cases, significantly different from the experimental master model. Most evident deviations were recorded in the sagittal (Y_2) and transversal plane (X_3) for all of the working casts. These were also the greatest distances among the measured abutments, so the differences were most likely to be observed. The measurement of all of the working casts was done by the principles of 3D measurement. Each surface of the abutments was measured with 50–100 surface points. The coordinates of surface points served as a base for measuring the geometry of the abutments. Due to a large number of data and easier analysis of measurement, the results were presented as a cross-section of the model in one plane, which in this case passed through the base of the abutments. This is why the results are presented as the classical 2D measurement, but the principles of measurement are related to the entire surface of the measured model and additional data can be withdrawn for each additional cross-section²⁵.

The impression material used in this study had a defined polymerization contraction of $\leq 0.2\%$, while expansion of gypsum was claimed to be 0.19% by the manufacturer. Expansion of gypsum would thus compensate for polymerization contraction of the impression material, but it should be noted that these values refer to the two sizes that are not equal, *ie* the thickness of the impression material in accordance with the height and width of the gypsum abutments²⁶. Thickness of the impression material varied from 1 to 3 mm from each side of the abutment, while the height and width of the abutments varied between 4.5 and 7.5 mm. In relation to this, expansion of gypsum should be a more dominant factor, which was proven by this study. Additionally, the influence of the micromechanical retention of the impression material to a custom tray should also be considered. In this case, the expansion of gypsum will be superimposed with the impression materials contraction towards the tray's walls, so that the combined effect will be presented by even wider abutments. As for the height of the abutments, where the upper surface was smaller than the side surface of the custom tray, in most cases the height of the abutments was smaller than that of the master model (Z_{1-6}). This can also be explained by impression materials contraction towards the walls. As the side surface of the tray had a bigger contact area than the upper one, the impression material was pulled down, which resulted in shorter abutments. These results are in accordance with other studies where tray adhesive was used in their research protocols^{27–29}.

The previously described process indicates that the silicone addition had a good retention with a custom tray made of epoxy resin by the RP technique. Although the RP technique is not widely used in the field of dentistry, it shows promise for manufacturing of dental devices. Its use in

everyday practice, as a rational method for fabrication of custom trays, requires advanced systems for intra- or extraoral scanning, together with an adequate software connected to an RP machine, which is currently a limiting factor. Additive technologies such as RP are mainly being used for the production of dental copings for fixed dental restoration, fabrication of surgical guides in implant dentistry and in reconstructive maxillofacial surgery^{30, 31}. As there is a large variety of materials that can be used for the production of custom trays with RP technology in different working regimes, these results are just a starting point and require additional investigation.

The analysis of convergence of axial surfaces showed that the largest deviations were observed in the third custom tray ($\alpha_1 = -0.18^\circ$), while deviations of the second tray ($\alpha_{1,2} = -0.11^\circ$) and the first tray ($\alpha_1 = -0.09^\circ$) were smaller. The angle of convergence was measured by scanning the axial surface and further software processing. Although small, deviations detected were oriented towards the increase of convergence. Convergence of the axial wall of the master model abutments was set to 6° (total of 12° when observing both axial planes), while gypsum abutments were detected to have more of a taper. The increase of the convergence angle reduces the overall surface of the abutment, which can influence the retention of the dental restoration³². While the width of the abutments was wider in the base cross-section, the axial surface has proven to have more taper. This could be explained by the increase of thickness of the impression material towards the upper base of the abutment and lower retention to the impression tray. Also, during removal of the impression the material deforms elastically. The resulting effect will be more pronounced in the axial surface, because of the overall increase of contact surface and direction of removal force away from the base of the abutment. This may all together explain the behaviour of the material to contract towards the walls of the tray in the base area, while slightly contracting inwards as the height progresses.

The results of this study show that all three custom trays performed satisfactory, but slightly better results were obtained with custom trays with 1 or 2 mm spacing. This is contrary to the claim that the thickness of the impression material should be at least 3 mm to prevent distortion of the material³³. Due to a problem of correct positioning of the impression tray when thickness of the material is low, the custom tray with 2 mm spacing should be recommended for use in the clinical practice. This is considered to be beneficial regarding the accuracy of the impression, ease of handling and reduction of the quantity of material. Making a precise impression is especially important when constructing long-span bridges, because the accuracy of fit is harder to achieve as the number of abutment teeth and the distance between them increases. In this case, custom trays should be recommended, because they provide uniform thickness of impression material that can influence the accuracy of working casts. The issue of impression material bulk and its effect on accuracy of working casts has been previously addressed. Plausible results were obtained up to 5 mm of the impression material^{14–18, 34, 35}.

Difficulty of comparison of our own results with other studies, lies in the complexity of the methodological procedure. Even comparison with studies that used the monophasic impression technique, as it was in this study, should be observed not only by input, but also by output parameters, which are obtained through the use of the measurement instrument. As most of the studies used different measurement procedures, a relevant overview is hard to achieve, so we will restrain from further data comparison.

Limitations of this study are related primarily to the method of measurement. Although CMM is an instrument of great accuracy and precision, it is necessary to know the geometry of the measurement object in order to obtain reliable results³. Because the measurement is done by a relatively small amount of surface points (in this study up to 100), the measurement object has to be clearly defined before the measurement takes place. Since the master model of known dimensions and shape was used, measuring in this study is characterized by considerable accuracy and precision.

Based on the obtained data, future studies would be based on determining of accuracy of the rest of the production process of dental restorations, including production of wax patterns and the casting procedure. Detection of flaws in each of the stages of the production procedure, will provide

useful guidelines for the dentists and dental technicians for the improvement of the quality of dental restorations.

Conclusion

The results of this study show that the impression material bulk of 1–3 mm could provide accurate working casts when using a monophasic impression technique. The increase of the distance between abutment teeth influences the accuracy of working casts. Custom trays produced by rapid prototyping can be successfully used for dental impressions. The experimental master model, combined with a CMM, is a reliable tool for assessment of dental impression accuracy.

Acknowledgements

The results presented in this paper were obtained in the framework of the project entitled “Research and development of modelling methods and approaches in manufacturing of dental recoveries with the application of modern technologies and computer aided systems” – TR 35020, financed by the Ministry of Education, Science and Technological Development of the Republic of Serbia.

R E F E R E N C E S

- Rosenstiel SF, Land MF, Fujimoto J. Contemporary fixed prosthodontics. St. Louis: Mosby Inc; 2006.
- Quaas S, Rudolph H, Luthardt RG. Direct mechanical data acquisition of dental impressions for the manufacturing of CAD/CAM restorations. *J Dent* 2007; 35(12): 903–8.
- Ender A, Mehl A. Accuracy of complete-arch dental impressions: a new method of measuring trueness and precision. *J Prosthet Dent* 2013; 109(2): 121–8.
- Trišković B, Budak I, Todorović A, Hodolić J, Puškar T, Jevremović D, et al. Application of Replica Technique and SEM in Accuracy Measurement of Ceramic Crowns. *Measur Sci Rev* 2012; 12(3): 90–7.
- Persson ASK, Odén A, Andersson M, Sandborgh-Englund G. Digitization of simulated clinical dental impressions: virtual three-dimensional analysis of exactness. *Dent Mater* 2009; 25(7): 929–36.
- Rodriguez JM, Bartlett DW. The dimensional stability of impression materials and its effect on in vitro tooth wear studies. *Dent Mater* 2011; 27(3): 253–8.
- Ceyhan JA, Johnson GH, Lepe X. The effect of tray selection, viscosity of impression material, and sequence of pour on the accuracy of dies made from dual-arch impressions. *J Prosthet Dent* 2003; 90(2): 143–9.
- Caputi S, Varvara G. Dimensional accuracy of resultant casts made by a monophasic, one-step and two-step, and a novel two-step putty/light-body impression technique: An in vitro study. *J Prosthet Dent* 2008; 99(4): 274–81.
- Luthardt RG, Kühmstedt P, Walter MH. A new method for the computer-aided evaluation of three-dimensional changes in gypsum materials. *Dent Mater* 2003; 19(1): 19–24.
- Brosky ME, Pesun IJ, Lowder PD, DeLong R, Hodges JS. Laser digitization of casts to determine the effect of tray selection and cast formation technique on accuracy. *J Prosthet Dent* 2002; 87(2): 204–9.
- Mishra S, Chowdhary R. Linear dimensional accuracy of a polyvinyl siloxane of varying viscosities using different impression techniques. *J Investig Clin Dent* 2010; 1(1): 37–46.
- Marković D, Puškar T, Hadžistević M, Potran M, Blažić L, Hodolić J. The dimensional stability of elastomeric dental impression materials. *Contemp Mater* 2012; 3(1): 105–10.
- Poniatowska M. Parameters for CMM Contact Measurements of Free-Form Surfaces. *Metrol Measur Sys* 2011; 18(2): 199–208.
- Nissan J, Gross M, Shifman A, Assif D. Effect of wash bulk on the accuracy of polyvinyl siloxane putty-wash impressions. *J Oral Rehabil* 2002; 29(4): 357–61.
- Kumar V, Aeran H. Evaluation of Effect of Tray Space on the Accuracy of Condensation Silicone, Addition Silicone and Polyether Impression Materials: An In Vitro Study. *J Indian Prosthodont Soc* 2012; 12(3): 154–60.
- Hoyos A. Influence of tray rigidity and material thickness on accuracy of polyvinyl siloxane impressions [thesis]. Gainesville, FL: Graduate School of the University of Florida; 2006.
- de Araujo PA, Jorgensen KD. Effect of material bulk and undercuts on the accuracy of impression materials. *J Prosthet Dent* 1985; 54(6): 791–4.
- Rajapur A, Dixit S, Hoshing C, Raikar SP. The influence of tray space and repeat pours on the accuracy of monophasic polyvinylsiloxane impression. *J Contemp Dent Pract* 2012; 13(6): 824–9.
- Mandikos MN. Polyvinyl siloxane impression materials: an update on clinical use. *Aust Dent J* 1998; 43(6): 428–34.
- Fehling AW, Hesby RA, Pelleu GB. Dimensional stability of autopolymerizing acrylic resin impression trays. *J Prosthet Dent* 1986; 55(5): 592–7.
- Sched RC, Weiss G. Woelfel's dental anatomy. Philadelphia: Lippincott Williams&Wilkins; 2012. p. 41.
- International Organization for Standardization. ISO/TS 17450-1. Geometrical product specification (GPS) – General concept – Part 1: Model for geometric specification and verification.

- cation. Geneva: International Organization for Standardization; 2002.
23. *Weckenmann A, Knauer M, Kunzmann H.* The Influence of Measurement Strategy on the Uncertainty of CMM-Measurements. *CIRP Annal Manufac Technol* 1998; 47(1): 451–4.
 24. *Wilhelm RG, Hocken R, Schwenke H.* Task Specific Uncertainty in Coordinate Measurement. *CIRP Annal Manufac Technol* 2001; 50(2): 553–63.
 25. *Chandran DT, Jagger DC, Jagger RG, Barbour ME.* Two- and three-dimensional accuracy of dental impression materials: effects of storage time and moisture contamination. *Biomed Mater Eng* 2010; 20(5): 243–9.
 26. *de Long R, Heinzen M, Hodges JS, Ko CC, Douglas WH.* Accuracy of a system for creating 3D computer models of dental arches. *J Dent Res* 2003; 82(6): 438–42.
 27. *Boulton JL, Gage JP, Vincent PF, Basford KE.* A laboratory study of dimensional changes for three elastomeric impression materials using custom and stock trays. *Aust Dent J* 1996; 41(6): 398–404.
 28. *Johnson GH, Craig RG.* Accuracy of four types of rubber impression materials compared with time of pour and a repeat pour of models. *J Prosthet Dent* 1985; 53(4): 484–90.
 29. *Lewinstein I.* The ratio between vertical and horizontal changes of impressions. *J Oral Rehabil* 1993; 20(1): 107–14.
 30. *Jevremovic DP, Puskar TM, Budak I, Vukelic DJ, Kojic V, Eggbeer D,* et al. An RE/RM approach to the design and manufacture of removable partial dentures with a biocompatibility analysis of the f75 Co-Cr-Slm alloy. *Mat Technol* 2012; 46(2): 123–9.
 31. *Wu M, Tinschert J, Augthun M, Wagner I, Schädlich-Stubenrauch J, Sahm PR,* et al. Application of laser measuring, numerical simulation and rapid prototyping to titanium dental castings. *Dent Mat* 2001;7(2):02–8.
 32. *Chan DC, Chan BH, Chung AK.* Mathematical modeling of molar tooth preparations for complete crowns. *J Dent* 2007; 35(11): 875–7.
 33. *Schaefer O, Schmidt M, Goebel R, Kuepper H.* Qualitative and quantitative three-dimensional accuracy of a single tooth captured by elastomeric impression materials: An in vitro study. *J Prosthet Dent* 2012; 108(3): 165–72.
 34. *Tjan AH, Nemetz H, Nguyen LTP, Contino R.* Effect of tray space on the accuracy of monophasic polyvinylsiloxane impressions. *J Prosthet Dent* 1992;8(1): 19–28.
 35. *Eames WB, Sieweke JC, Wallace SW, Rogers LB.* Elastomeric impression materials: effect of bulk on accuracy. *J Prosthet Dent* 1979; 41(3): 304–7.

Received on January 5, 2015.

Revised on March 17, 2015.

Accepted on May 19, 2015.

Online First May, 2016.